


Qualitätskontrollzertifikat / Quality Control Certificate

Kitcharge / Lot EQ0230 IFU-Version 105-28
 Verw. bis / Exp. 2027-10-31 **!New!**

21.11.2025

Prüfdatum /

Date of control

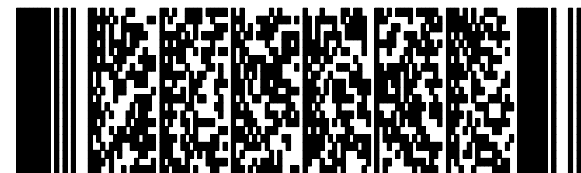

Verwendete Reagenzien / Reagents used	Lot	Standard	Standard Kurve / Standard curve
Teststreifen / Antigen coated strips	ECP0473	Ref.- Werte / Ref. Values	Parameter A 0,007 B 0,991 C 5,767 D 3,157
Standardserum / Standard serum	ECQ0509	OD 0,85	
Negativ Kontrolle / Negative control	ECQ0508		
Konjugat / Conjugate	KJQ091+++	Units 116 U/ml	
Quantifizierungsgrenzen / Limits of quantification		U/ml 10 - 1000	
Grenzwertbereich / Borderline range		U/ml 20 - 30	

OD Bereich / OD Range 405 nm, Standardserum / Standard serum										Interpretation
0,43 - 0,47	0,48 - 0,52	0,53 - 0,57	0,58 - 0,63	0,64 - 0,68	0,69 - 0,73	0,74 - 0,79	0,80 - 0,84	0,85	U/ml	
< 0,11	< 0,12	< 0,13	< 0,14	< 0,16	< 0,17	< 0,18	< 0,19	< 0,20	< 20,0	neg
0,11 - 0,15	0,12 - 0,16	0,13 - 0,18	0,14 - 0,20	0,16 - 0,22	0,17 - 0,23	0,18 - 0,25	0,19 - 0,27	0,20 - 0,28	20,0 - 30,0	gw / borderline
> 0,15	> 0,16	> 0,18	> 0,20	> 0,22	> 0,23	> 0,25	> 0,27	> 0,28	> 30,0	pos

OD Bereich / OD Range 405 nm, Standardserum / Standard serum										Interpretation
U/ml	0,85	0,86 - 0,92	0,93 - 1,00	1,01 - 1,07	1,08 - 1,15	1,16 - 1,22	1,23 - 1,30	1,31 - 1,37	1,38 - 1,45	
< 20,0	< 0,20	< 0,21	< 0,23	< 0,24	< 0,26	< 0,28	< 0,30	< 0,31	< 0,33	neg
20,0 - 30,0	0,20 - 0,28	0,21 - 0,29	0,23 - 0,32	0,24 - 0,34	0,26 - 0,37	0,28 - 0,39	0,30 - 0,42	0,31 - 0,44	0,33 - 0,47	gw / borderline
> 30,0	> 0,28	> 0,29	> 0,32	> 0,34	> 0,37	> 0,39	> 0,42	> 0,44	> 0,47	pos

Formeln für spezielle Auswertesysteme
 Special case formulas

OD = 0,333 x MV(STD) entspricht oberem cut-off/ corresponds to upper cut-off
 OD = 0,232 x MV(STD) entspricht unterem cut-off/ corresponds to lower cut-off
 Concentration= exp(5,767-ln(3,15/(MV(Sample) x0,85/ MV(STD)-0,007)-1)/0,991)

30 Institut Virion\Serion GmbH
 20 Friedrich-Bergius-Ring 19
 D-97076 Würzburg

**Zusätzliche Barcodes mit Formeln für / Additional Barcodes with formulas for
Revelation™ DSX / DS-Matrix™****4PS- Formel / 4PS-formula**
$$\exp(5.767 - \ln(3.150 / (\text{Sample}^{0.850} / S - 0.007) - 1) / 0.991)$$
**Gültigkeitsbereich / Validity Range**
$$0.425 \leq S1 \leq 1.445$$
**If OD Sample < Parameter A**
$$\text{if } Ti < (0.007 * (S1 / 0.850)) \text{ then } Ti = (0.007 + 0.001) * (S1 / 0.850)$$
**If OD Sample > Parameter D**
$$\text{if } Ti > (3.157 * (S1 / 0.850)) \text{ then } Ti = (3.157 - 0.001) * (S1 / 0.850)$$
**If OD Negative control < Parameter A**
$$\text{if } NC1 < (0.007 * (S1 / 0.850)) \text{ then } NCi = (0.007 + 0.001) * (S1 / 0.850)$$
